


RIQAS

RANDOX INTERNATIONAL QUALITY ASSESSMENT SCHEME

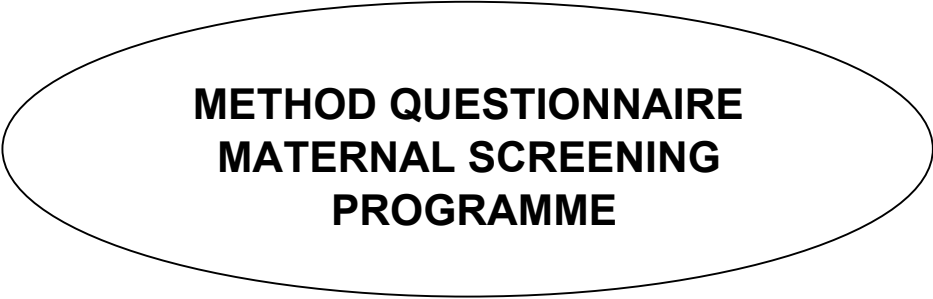

**METHOD QUESTIONNAIRE
MATERNAL SCREENING
PROGRAMME**

This document must be retained by participant

REGISTRATION INSTRUCTIONS & RIQAS POLICIES

CRITERIA FOR PARTICIPATION

This programme is available to any laboratory running the Maternal Screening assays listed in this document. Quantitative results will be accepted on this programme.

INTRODUCTION

Method questionnaires are available for all routine *RIQAS* Programmes. They are designed to allow you to register for this *RIQAS* Programme and to inform you of *RIQAS* protocols and policies. It is important that you read and understand all the information in these introductory pages. If you have any questions or concerns about any of the information presented in this document, please contact *RIQAS* either directly or through your local Randox Laboratories representative.

REGISTRATION INSTRUCTIONS

1. METHOD QUESTIONNAIRE:- To be retained by participant

This method questionnaire should be completed and retained by you for your records. Please ensure that you complete the method questionnaire in full. Your details will help us to classify your results correctly and thus provide you with useful statistical data.

Following these introductory pages you will find:

The method questionnaire, which indicates the method codes available for each parameter along with the standard *RIQAS* unit.

On the method questionnaire, for each parameter you wish to run, please tick the method appropriate to you, then state your instrument code, reagent code, and the units that you use in your laboratory if they are different from the *RIQAS* standard units. If codes are not available for your assay, please state the details of your method clearly in the section at the end of the enrolment document.

Once your method questionnaire has been completed, you must transfer the information onto your enrolment document.

2. ENROLMENT DOCUMENT:- To be returned to *RIQAS*

Please be aware that it may take up to 3 weeks to process enrolment documents.

A. LABORATORY REFERENCE NUMBER

Each participant is assigned a **laboratory reference number** which consists of a **participant number** which is unique to your laboratory and a **registration letter** which is assigned for each new registration we receive from you. If you are a current or previous participant, please state your **participant number** on the enrolment document. If you do not have a Laboratory Reference Number, this will be generated by *RIQAS* when you register for the first time.

B. ORDER NUMBER

If you are a UK or Irish participant, please state your official order number in the boxes provided. Other participants may order directly from their local Randox Laboratories representative.

C. CYCLE/PRODUCT REQUIREMENTS

Please tick the cycles you wish to subscribe for. If there is more than one kit/product offered for the programme, please also tick the kit you wish to subscribe for.

D. CONTACT DETAILS

It is important to state the name and full address details of the Quality Assessment Officer or contact person who will receive all correspondence and routine reports during the cycle. Please also state the company name of the Randox representative who is supplying you with the *RIQAS* product under 'Randox Representative'.

E. *RIQAS* Net

RIQAS Net is a web-based online method for result entry/method changes/viewing of released reports. Reports will be sent to up to 3 email addresses as PDF files. Internet access and login details are required for *RIQAS* Net and Adobe Reader is required for viewing reports. If you wish to use *RIQAS* Net please indicate this by ticking the box on the enrolment document. Your login information and password will be supplied by *RIQAS*. Your login information will be based on the 1st email address you supply on your enrolment document. A PDF copy of the report will be sent to this address and can also be sent to 2 other email addresses. These addresses should be stated on your enrolment document.

F. PDF reports

Reports can now be sent as PDF files as an alternative to paper reports. These files can be sent to up to 3 email addresses. If you wish to receive PDF reports please indicate this by ticking the box on the enrolment document and include the email addresses to which the reports should be sent. Adobe Reader is required to view the reports.

G. GROUP REPORTS

It is possible to enrol **multiple instruments** within your laboratory. **Kindly complete separate enrolment documents for each instrument.** A **complementary instrument group report** is supplied if you have returned results for more than one registration of the same programme. If you intend to enrol laboratories at different sites or if you are part of a group of laboratories, an **inter-laboratory group report for each sample** can be supplied on receipt of a completed authorisation form from each registered laboratory. Please contact *RIQAS* for a copy of the official inter-laboratory authorisation form.

H. REGISTRATION OF METHODS

Complete the 'Registration of Methods' section for all required parameters using the codes you selected on your method questionnaire. If no code is available for your assay, please state the details of your method clearly in the section at the end of the enrolment document.

For Ortho-Clinical Diagnostics VITROS registrations, please state the 2 digit slide Generation number for each analyte.

If units other than the standard RIQAS units are used, please specify these in the boxes supplied.

Once completed, the enrolment document should be sent to RIQAS for registration.

NOTE: IF A REGISTERED PARTICIPANT DOES NOT PARTICIPATE FOR A CYCLE, THEY WILL BE EXPECTED TO COMPLETE NEW ENROLMENT DOCUMENTS IN ORDER TO RE-JOIN THE PROGRAMME.

I. CHANGES DURING A CYCLE

Please inform RIQAS of any change to contact details as soon as possible. It is also possible to change your unit, method, instrument or reagent classification during a cycle.

Participants who use return sheets: Each Results Return Sheet has a section for method changes. Please state your new classification codes at the bottom of your next return sheet. We assume that your new classification will be in routine use from the date on the return sheet unless you tell us otherwise. If you have added or deleted a parameter, changed your unit or Vitros slide generation number, an updated return sheet will be forwarded to you. It is important that you discard your old return sheet and use only your updated copy for future returns.

Participants who use RIQAS Net: Changes can be made in the Method Changes section of the Data Entry menu. A list of your registered laboratory reference numbers will appear on screen. Select the laboratory reference number for which you would like to change the assay details. A current list of assay details will appear. Click on the appropriate parameter and the assay details will appear. To change the details click the arrow box on the appropriate details and select a new one. Save the changes and submit them to RIQAS. Changes will not be instantaneously updated. On receipt of method changes RIQAS staff will manually process and update your assay details which will then be uploaded onto RIQAS Net. It is possible to submit results and method changes at the same time as method changes will be made before results are submitted.

LABORATORY REFERENCE NUMBERS & RETURN SHEETS

On receipt of your enrolment document RIQAS will generate a **Laboratory Reference Number** for your laboratory and additional numbers for associated laboratories or multiple instruments if requested. If you are registering for the first time you will be sent RIQAS literature, which will enable you to understand the RIQAS process and interpret your reports.

Participants using RIQAS Net will receive an email containing their login information. Once you have successfully logged in to RIQAS Net you will see your various laboratory reference numbers for each registered programme.

Participants who do not use RIQAS Net will be sent a master return sheet which is specific for your registered parameters and units. You should photocopy this sheet as required and use it to return results to RIQAS.

ORDERING RIQAS PRODUCTS

Please ensure that your order is placed with your local Randox representative **at least 6-8 weeks** before the cycle starts. This will ensure sufficient time to process and despatch your kit(s) to you. Participants from UK or Ireland may order products directly from RIQAS with an official order number. Orders received within 6 weeks of the start of the cycle will be processed, but RIQAS cannot guarantee delivery in time for the first sample. Current prices of RIQAS products are available from your local Randox Laboratories representative.

It may be possible to order RIQAS products during a cycle, subject to availability. Please contact your local Randox representative for more information.

SHIPPING AND RECEIPT OF RIQAS PRODUCTS

Provided that you have ordered sufficiently in advance, your RIQAS kit(s) will be shipped to you to arrive before the analysis date of the first sample in the kit. If you do not receive your kit(s) before this time, please contact your local Randox representative.

On receipt of your RIQAS kit, please check that:

- a) it is the product you ordered
- b) the tamper-proof label has not been broken
- c) the kit contains detailed Instructions For Use (IFU), including material characteristics, preparation, stability, storage and safety
- d) the correct number of samples are present as indicated on the IFU
- e) the samples have the appearance as indicated on the IFU and that none of them are damaged

Please notify your local Randox representative immediately if any of these are incorrect.

Please ensure that the product is immediately stored according to the recommendations on the package labelling.

ASSAY OF SAMPLES & RETURN OF RESULTS

Carefully read the instructions stated on the Instructions for Use (IFU) prior to preparation and assay of RIQAS samples. The RIQAS samples should be assayed at the recommended time specified on the IFU. Following appropriate preparation, samples should be treated as routine, unless otherwise stated on the IFU. Please assay the samples on or before the recommended date for analysis and forward your results to RIQAS by no later than **17:00 GMT on the FINAL DATE**, as indicated in the IFU. If returning results on return sheet, it is most important that your Laboratory Reference Number(s), cycle number, sample number and FINAL DATE for return of results are clearly written at the top of the return sheet. If you wish to fax your results please transmit them 3 working days before the FINAL DATE to + 44 (0) 28 9445 4398. You may also e-mail your results to mail@riqas.com. Please contact RIQAS for a RESULT RETURN SHEET template.

LATE AND CORRECTED RESULTS

In keeping with the objectives of EQA schemes, participants should be aware that collusion and falsification of results is considered to be unethical and constitutes scientific fraud. While *RIQAS* permits the submission of late or corrected results under the circumstances described below, routine reports are clearly marked to indicate late and corrected results.

LATE RESULTS

Results received after the FINAL DATE will be processed retrospectively. Participants will still receive their report which will record late results as "NO RESULTS" until reprocessing is complete. Please ensure that any late results you wish to submit reach us by no later than the final date of the following sample. Any results received after this date will not be entered.

CORRECTED RESULTS

Participants will be permitted to submit corrected results up to 4 weeks after the final date of the sample. While a new report will not be issued, corrected results will be processed retrospectively and results can be viewed on subsequent reports.

DESPATCH OF REPORTS

Results will normally be processed within 2 days of the FINAL DATE. Reports sent by PDF reports will be sent as soon as the results have been processed and for those registered for *RIQAS* Net the PDF reports will be available on *RIQAS* Net shortly after. Printed reports usually take a further 1-3 days to print and despatch.

CERTIFICATES OF PARTICIPATION

Complimentary certificates of participation for each *RIQAS* programme are available to participants at the **end of the current cycle**, provided that at **least 50%** of results have been returned. The certificate will specify the cycle, programme and the LABORATORY / HOSPITAL NAME specified in the address details of the enrolment document. Modified certificates may be requested through your local Randox representative. At the end of a cycle, a list of all eligible labs will be sent to the local Randox representative who will confirm the Laboratory/Hospital Name. This list will be returned to the *RIQAS* department and certificates printed according to the details sent by the local Randox representative. If any modifications or additions are required after this list has been finalised an administration fee will be charged.

CONFIDENTIALITY

Participation in any *RIQAS* programme is considered to be strictly confidential. Any data transfer or correspondence with participants, either directly or via local Randox representative, will be deemed confidential. Participants should be aware that their laboratory accreditation bodies have the right to request an assessment of a participant's performance. Where regulatory authorities are to be provided with a participant's results, participants will be notified.

PERFORMANCE SURVEILLANCE OF UK LABS

RIQAS is obligated to identify and report persistent poor performing UK labs to the National Quality Assessment Advisory Panel. Poor performers are identified as those failing to meet performance criteria agreed with NQAAP. The performance criteria is specified in all performance surveillance correspondence with participants, and is also available on request. Participants are initially informed of poor performance by letter. Failure to improve performance will prompt details to be forwarded to NQAAP. All information sent to participants and NQAAP is strictly confidential. Please contact *RIQAS* if you require further information on Performance Surveillance.

PARTICIPANT FEEDBACK & RIGHT TO APPEAL

In order to ensure that *RIQAS* provides an appropriate and satisfying service, all participants will be provided with a feed-back questionnaire towards the end of a cycle. We would invite you to contact us at any time during the cycle, should you have any requests for additional programmes or parameters or comments regarding existing programmes.

RIQAS makes every effort to ensure that the samples provided are clinically challenging to as many laboratory systems as possible. For details, please contact *RIQAS* either directly or through your local Randox representative.

Should the need arise, participants may appeal against the interpretation of their results or assessment of their performance through correspondence with the local Randox Laboratories representative or by contacting *RIQAS* directly.

SUB-CONTRACTING

RIQAS sub-contracts aspects of the scheme. *RIQAS* accepts responsibility for the sub-contractors' work and protocols are in place to ensure that sub-contractors are deemed competent.

OUR COMPETENCE AS A PROFICIENCY TESTING PROVIDER

On request, *RIQAS* is willing to co-operate with participants seeking evidence of our competence as a proficiency testing provider or information on the design and implementation of *RIQAS* Programmes.

DEVIATION FROM EXISTING POLICIES/SERVICE

If there is any deviation from the existing policies or service, participants will be notified either directly or via their local Randox representative.

THIS PROGRAMME HAS NOT YET BEEN ACCREDITED
TO ILAC G13:08/2007

Please contact *RIQAS* at

Tel: +44 (0) 28 9445 4399

Fax: +44 (0) 28 9445 4398

E-Mail mail@riqas.com

RIQAS Scheme Co-ordinator: Stephen Doherty

RANDOX LABORATORIES LTD., Ardmore, Diamond Road, Crumlin, Co. Antrim, United Kingdom, BT29 4QY

Revised July 2010

MATERNAL SCREENING PROGRAMME

METHOD QUESTIONNAIRE

AFP - kU/l

CODE	METHOD
AFARC	<input type="checkbox"/> Abbott Architect
AFABX	<input type="checkbox"/> Abbott Axsym/Axsym Plus
AFSAN	<input type="checkbox"/> Beckman Access/LXi725
AFDXI	<input type="checkbox"/> Beckman DxI800
AFBIV	<input type="checkbox"/> bioMerieux Vidas/Mini Vidas
AFBMR	<input type="checkbox"/> Bio-rad Microplate Reader
AFBRR	<input type="checkbox"/> Brahms Krytor
AFCII	<input type="checkbox"/> CIS IRMA
AFETI	<input type="checkbox"/> Diasorin ETI-MAX 3600
AFLIA	<input type="checkbox"/> Diasorin Liason
AFDRE	<input type="checkbox"/> DRG Elisa
AFGM	<input type="checkbox"/> Gamma Counter
AFHUM	<input type="checkbox"/> Human Humanreader
AFIMI	<input type="checkbox"/> Immunotech IRMA
AFOR	<input type="checkbox"/> Organon Reader 530
AFVEC	<input type="checkbox"/> Ortho Vitros, 3600/5600/ECi
AFC6	<input type="checkbox"/> Roche Cobas 6000
AFEYS	<input type="checkbox"/> Roche Elecsys 2010/1010
AFRME	<input type="checkbox"/> Roche Modular E170
AFCC	<input type="checkbox"/> Siemens/Bayer ACS 180
AFcen	<input type="checkbox"/> Siemens/Bayer Advia Centaur
AFDD	<input type="checkbox"/> Siemens/Dade Dimension
AFDS	<input type="checkbox"/> Siemens/Dade Stratus
AFDPI	<input type="checkbox"/> Siemens/DPC Immulite 1000
AFDP2	<input type="checkbox"/> Siemens/DPC Immulite 2000/2500
AFSF	<input type="checkbox"/> Stat Fax Elisa Readers
AFSTR	<input type="checkbox"/> Stratec Immunotech
AFTS	<input type="checkbox"/> Tecan Sunrise
AFDEL	<input type="checkbox"/> Wallac Delfia Xpress/Autodelfia
AFWW	<input type="checkbox"/> Wallac Wizard
AFZEN	<input type="checkbox"/> Zentech ELISA
AFO	<input type="checkbox"/> Other methods

OTHER UNITS SPECIFY

HCG Free Beta - U/l

CODE	METHOD
HCBARC	<input type="checkbox"/> Abbott Architect i2000/8200
HCBABX	<input type="checkbox"/> Abbott Axsym/Axsym Plus
HCBSAN	<input type="checkbox"/> Beckman Access
HCBDXI	<input type="checkbox"/> Beckman DxI800
HCBBIV	<input type="checkbox"/> bioMerieux Vidas Mini Vidas
HCBRR	<input type="checkbox"/> Brahms Krytor
HCBCII	<input type="checkbox"/> CIS IRMA
HCBETI	<input type="checkbox"/> Diasorin ETI-MAX 3600
HCBLIA	<input type="checkbox"/> Diasorin Liaison
HCBDR	<input type="checkbox"/> DRG Elisa
HCBHUM	<input type="checkbox"/> Human Humanreader
HCBIMI	<input type="checkbox"/> Immunotech IRMA
HCBOR	<input type="checkbox"/> Organon Reader 530
HCBVEC	<input type="checkbox"/> Ortho Vitros, 3600/5600/ECi
HCBC6	<input type="checkbox"/> Roche Cobas 6000
HCBEYS	<input type="checkbox"/> Roche Elecsys 2010/1010
HCBRME	<input type="checkbox"/> Roche Modular E170
HCBC	<input type="checkbox"/> Siemens/Bayer ACS 180
HCBCEN	<input type="checkbox"/> Siemens/Bayer Advia Centaur
HCBDD	<input type="checkbox"/> Siemens/Dade Dimension/RxL
HCBDS	<input type="checkbox"/> Siemens/Dade Stratus
HCBDP1	<input type="checkbox"/> Siemens/DPC Immulite 1000
HCBDP2	<input type="checkbox"/> Siemens/DPC Immulite 2000/2500
HCBSF	<input type="checkbox"/> Stat Fax Elisa Readers
HCBSTR	<input type="checkbox"/> Stratec Immunotech
HCBTS	<input type="checkbox"/> Tecan Sunrise
HCBDEL	<input type="checkbox"/> Wallac Delfia/Delfia Express/Autodelfia
HCBWW	<input type="checkbox"/> Wallac Wizard
HCBZEN	<input type="checkbox"/> Zentech ELISA
HCBO	<input type="checkbox"/> Other

OTHER UNITS SPECIFY

MATERNAL SCREENING PROGRAMME

METHOD QUESTIONNAIRE

HCG Total - U/I

CODE	METHOD
HCTARC	<input type="checkbox"/> Abbott Architect I2000/8200
HCTABX	<input type="checkbox"/> Abbott AxSYM/AxSYM Plus
HCTSAN	<input type="checkbox"/> Beckman Access
HCTAU	<input type="checkbox"/> Beckman Coulter AU 3000i
HCTDXI	<input type="checkbox"/> Beckman DxI800
HCTBIV	<input type="checkbox"/> bioMerieux Vidas/Mini Vidas
HCTBRR	<input type="checkbox"/> Brahms Krytor
HCTETI	<input type="checkbox"/> Diasorin ETI-MAX 3600
HCTLIA	<input type="checkbox"/> Diasorin Liaison
HCTIMI	<input type="checkbox"/> Immunotech IRMA
HCTVEC	<input type="checkbox"/> Ortho Vitros, 3600/5600/ECi
HCTRCE	<input type="checkbox"/> Roche Cobas e411
HCTEYS	<input type="checkbox"/> Roche Elecsys 2010/1010
HCTRME	<input type="checkbox"/> Roche Modular E170
HCTCC	<input type="checkbox"/> Siemens/Bayer ACS 180/180 SE
HCTCEN	<input type="checkbox"/> Siemens/Bayer Advia Centaur/CP
HCTDD	<input type="checkbox"/> Siemens/Dade Dimension/RxL
HCTDST	<input type="checkbox"/> Siemens/Dade Stratus
HCTDPI	<input type="checkbox"/> Siemens/DPC Immulite 1000
HCTDP2	<input type="checkbox"/> Siemens/DPC Immulite 2000/2500
HCSF	<input type="checkbox"/> Stat Fax Elisa Readers
HCTSTR	<input type="checkbox"/> Stratec Immunotech
HCTDEL	<input type="checkbox"/> Wallac Delfia/Delfia Express/Autodelfia
HCTWW	<input type="checkbox"/> Wallac Wizard
HCTO	<input type="checkbox"/> Other

OTHER UNITS SPECIFY

INHIBIN A - kU/I

CODE	METHOD
INAARC	<input type="checkbox"/> Abbott Architect I2000/ 8200
INAABX	<input type="checkbox"/> Abbott AxSYM/AxSYM Plus
INAAE	<input type="checkbox"/> Active Inhibin A ELISA
INASAN	<input type="checkbox"/> Beckman Access
INADSX	<input type="checkbox"/> Beckman DSX
INADXI	<input type="checkbox"/> Beckman DxI800
INABIV	<input type="checkbox"/> bioMerieux Vidas/Mini Vidas
INABRR	<input type="checkbox"/> Brahms Krytor
INAETI	<input type="checkbox"/> Diasorin ETI-MAX 3600
INALIA	<input type="checkbox"/> Diasorin Liaison
INAIMI	<input type="checkbox"/> Immunotech IRMA
INAVEC	<input type="checkbox"/> Ortho Vitros, 3600/5600/ECi
INAEYS	<input type="checkbox"/> Roche Elecsys 2010/1010
INARME	<input type="checkbox"/> Roche Modular E170
INACC	<input type="checkbox"/> Siemens/Bayer ACS 180/180 SE
INACEN	<input type="checkbox"/> Siemens/Bayer Advia Centaur
INADS	<input type="checkbox"/> Siemens/Dade Stratus
INADD	<input type="checkbox"/> Siemens/Dade Dimension
INADPI	<input type="checkbox"/> Siemens/DPC Immulite 1000
INADP2	<input type="checkbox"/> Siemens/DPC Immulite 2000/2500
INASF	<input type="checkbox"/> Stat Fax Elisa Readers
INASTR	<input type="checkbox"/> Stratec Immunotech
INADEL	<input type="checkbox"/> Wallac Delfia/Delfia Express/Autodelfia
INAWW	<input type="checkbox"/> Wallac Wizard
INAO	<input type="checkbox"/> Other

OTHER UNITS SPECIFY

MATERNAL SCREENING PROGRAMME

METHOD QUESTIONNAIRE

PAPP-A - U/I

CODE	METHOD
PPAARC	<input type="checkbox"/> Abbott Architect I2000/8200
PPAABX	<input type="checkbox"/> Abbott Axsym/Axsym Plus
PPSAN	<input type="checkbox"/> Beckman, Access
PPADX1	<input type="checkbox"/> Beckman DxI800
PPABIV	<input type="checkbox"/> bioMerieux Vidas/Mini Vidas
PPABRR	<input type="checkbox"/> Brahms Krytor
PPAETI	<input type="checkbox"/> Diasorin ETI-MAX 3600
PPALIA	<input type="checkbox"/> Diasorin Liaison
PPDRE	<input type="checkbox"/> DRG Elisa
PPAIMI	<input type="checkbox"/> Immunotech IRMA
PPAVEC	<input type="checkbox"/> Ortho Vitros, 3600/5600/ECi
PPAEYS	<input type="checkbox"/> Roche Elecsys 2010/1010
PPARME	<input type="checkbox"/> Roche Modular E170
PPACC	<input type="checkbox"/> Siemens/Bayer ACS 180/180 SE
PPACEN	<input type="checkbox"/> Siemens/Bayer Advia Centaur
PPADD	<input type="checkbox"/> Siemens/Dade Dimension
PPADS	<input type="checkbox"/> Siemens/Dade Stratus
PPADPI	<input type="checkbox"/> Siemens/DPC Immulite 1000
PPADP2	<input type="checkbox"/> Siemens/DPC Immulite 2000/2500
PPASF	<input type="checkbox"/> Stat Fax Elisa Readers
PPASTR	<input type="checkbox"/> Stratec Immunotech
PPADEL	<input type="checkbox"/> Wallac Delfia/Delfia Express/Autodelfia
PPAWW	<input type="checkbox"/> Wallac Wizard
PPAZEN	<input type="checkbox"/> Zentech ELISA
PPAO	<input type="checkbox"/> Other

OTHER UNITS SPECIFY

UNCONJUGATED ESTRIOL - nmol/l

CODE	METHOD
UE3ARC	<input type="checkbox"/> Abbott Architect I2000/8200
UE3ABX	<input type="checkbox"/> Abbott Axsym/Axsym Plus
UE3SAN	<input type="checkbox"/> Beckman Access
UE3DXI	<input type="checkbox"/> Beckman DxI800
UE3BIV	<input type="checkbox"/> bioMerieux Vidas/Mini Vidas
UE3BRR	<input type="checkbox"/> Brahms Krytor
UE3ETI	<input type="checkbox"/> Diasorin ETI-MAX 3600
UE3LIA	<input type="checkbox"/> Diasorin Liaison
UE3DRE	<input type="checkbox"/> DRG Elisa
UE3DSL	<input type="checkbox"/> DSL gammacounter
UE3HUP	<input type="checkbox"/> Human Plate
UE3IMI	<input type="checkbox"/> Immunotech IRMA
UE3OR	<input type="checkbox"/> Organon Reader 530
UE3VEC	<input type="checkbox"/> Ortho Vitros, 3600/5600/ECi
UE3EYS	<input type="checkbox"/> Roche Elecsys 2010/1010
UE3RME	<input type="checkbox"/> Roche Modular E170
UE3CC	<input type="checkbox"/> Siemens/Bayer ACS 180/180 SE
UE3CEN	<input type="checkbox"/> Siemens/Bayer Advia Centaur
UE3DD	<input type="checkbox"/> Siemens/Dade Dimension
UE3DS	<input type="checkbox"/> Siemens/Dade Stratus
UE3DPI	<input type="checkbox"/> Siemens/DPC Immulite 1000
UE3DP2	<input type="checkbox"/> Siemens/DPC Immulite 2000/2500
UE3SF	<input type="checkbox"/> Stat Fax Elisa Readers
UE3STR	<input type="checkbox"/> Stratec Immunotech
UE3TS	<input type="checkbox"/> Tecan Sunrise
UE3DEL	<input type="checkbox"/> Wallac Delfia/Delfia Express/Autodelfia
UE3WW	<input type="checkbox"/> Wallac Wizard
UE3ZEN	<input type="checkbox"/> Zentech ELISA
UE3O	<input type="checkbox"/> Other

OTHER UNITS SPECIFY